


Mass Spectrum

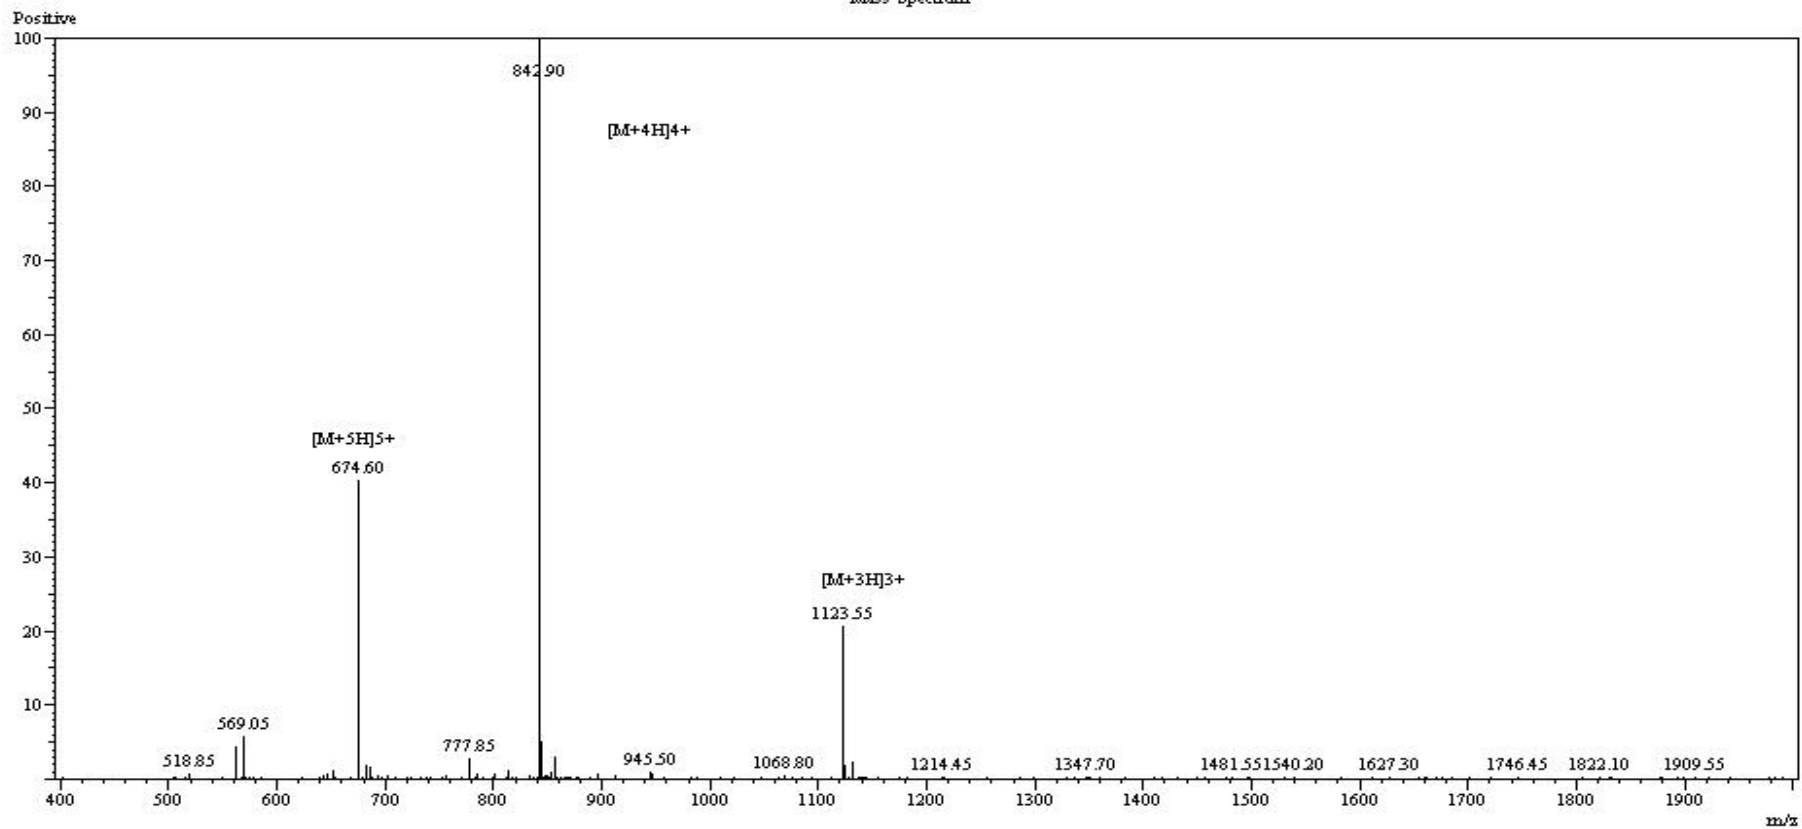

Sample Information

Date and Time : 2017-02-23 15:44:57  
User : SHAO  
Sample : 488704  
Inj. Volume : 1  
MW : 3367.2  
Lot No. : P170116-CQ488704

Probe: ESI  
Nebulizer Gas Flow: 1.5L/min  
CDL: -20.0v  
CDL Temp: 250°C  
Block Temp: 200°C

Probe bias: -3.5kv  
Detector: 1.0kv  
T. Flow: 0.2ml/min  
B. conc: 50%H2O/50%ACN