


Mass Spectrum

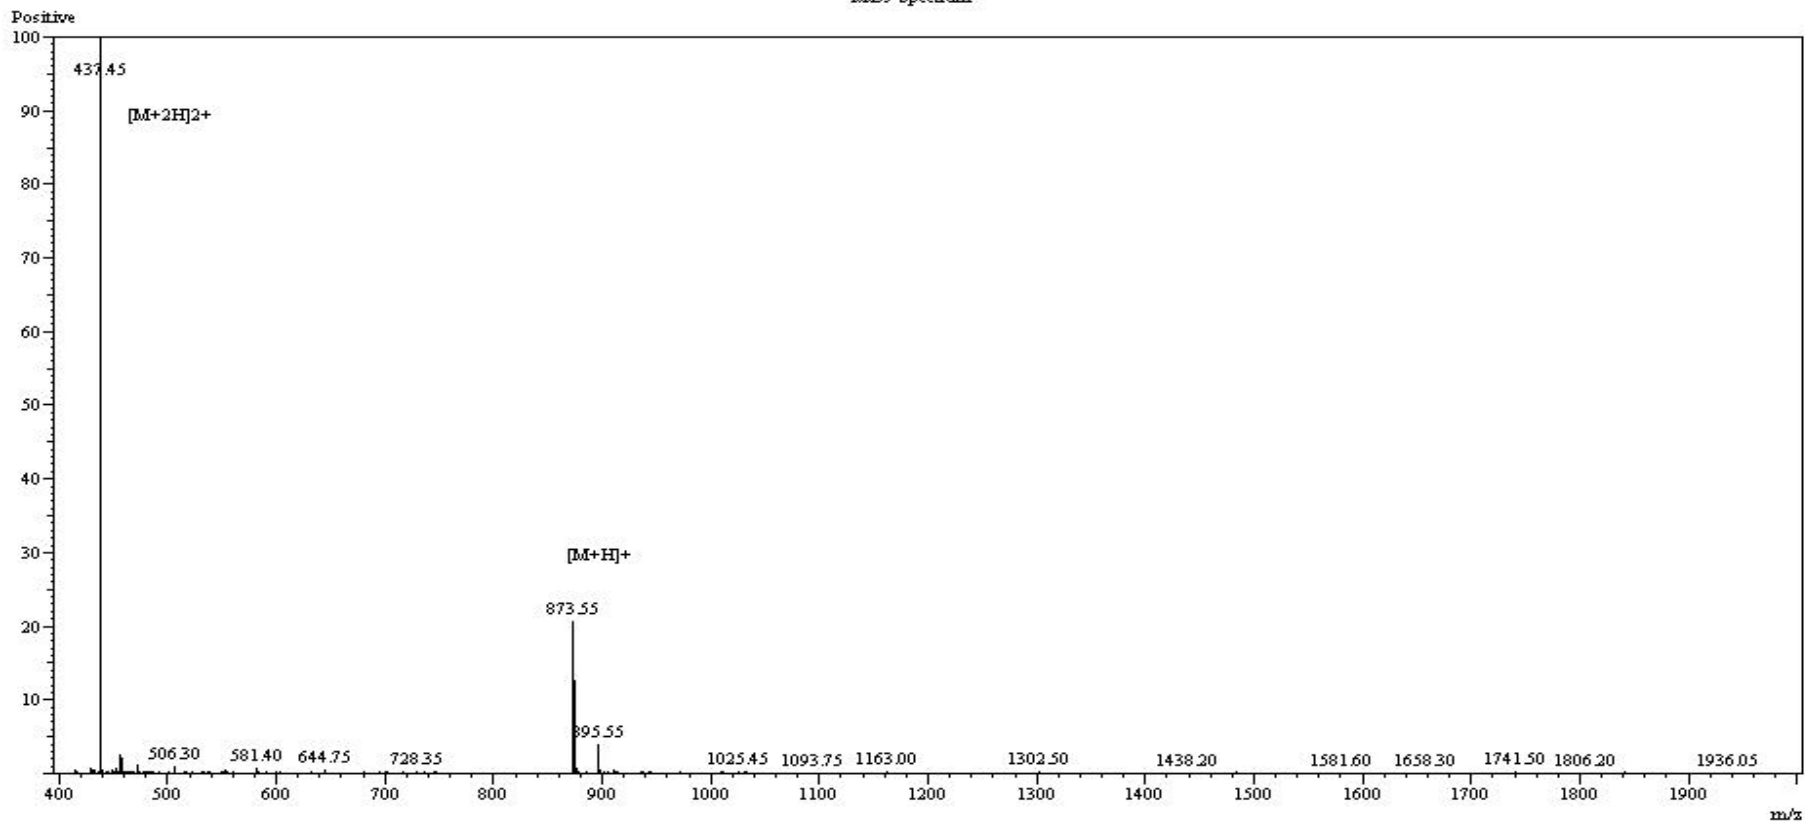

Sample Information

Date and Time : 2017-04-21 15:55:52
User : CHAO
Sample : 055254 055254
Inj. Volume : 1
MW : 873.04

Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp: 250°C
Block Temp: 200°C

Probe bias: -3.5kv
Detector: 1.0kv
T. Flow: 0.2ml/min
B. conc: 50%H2O/50%ACN