


Mass Spectrum

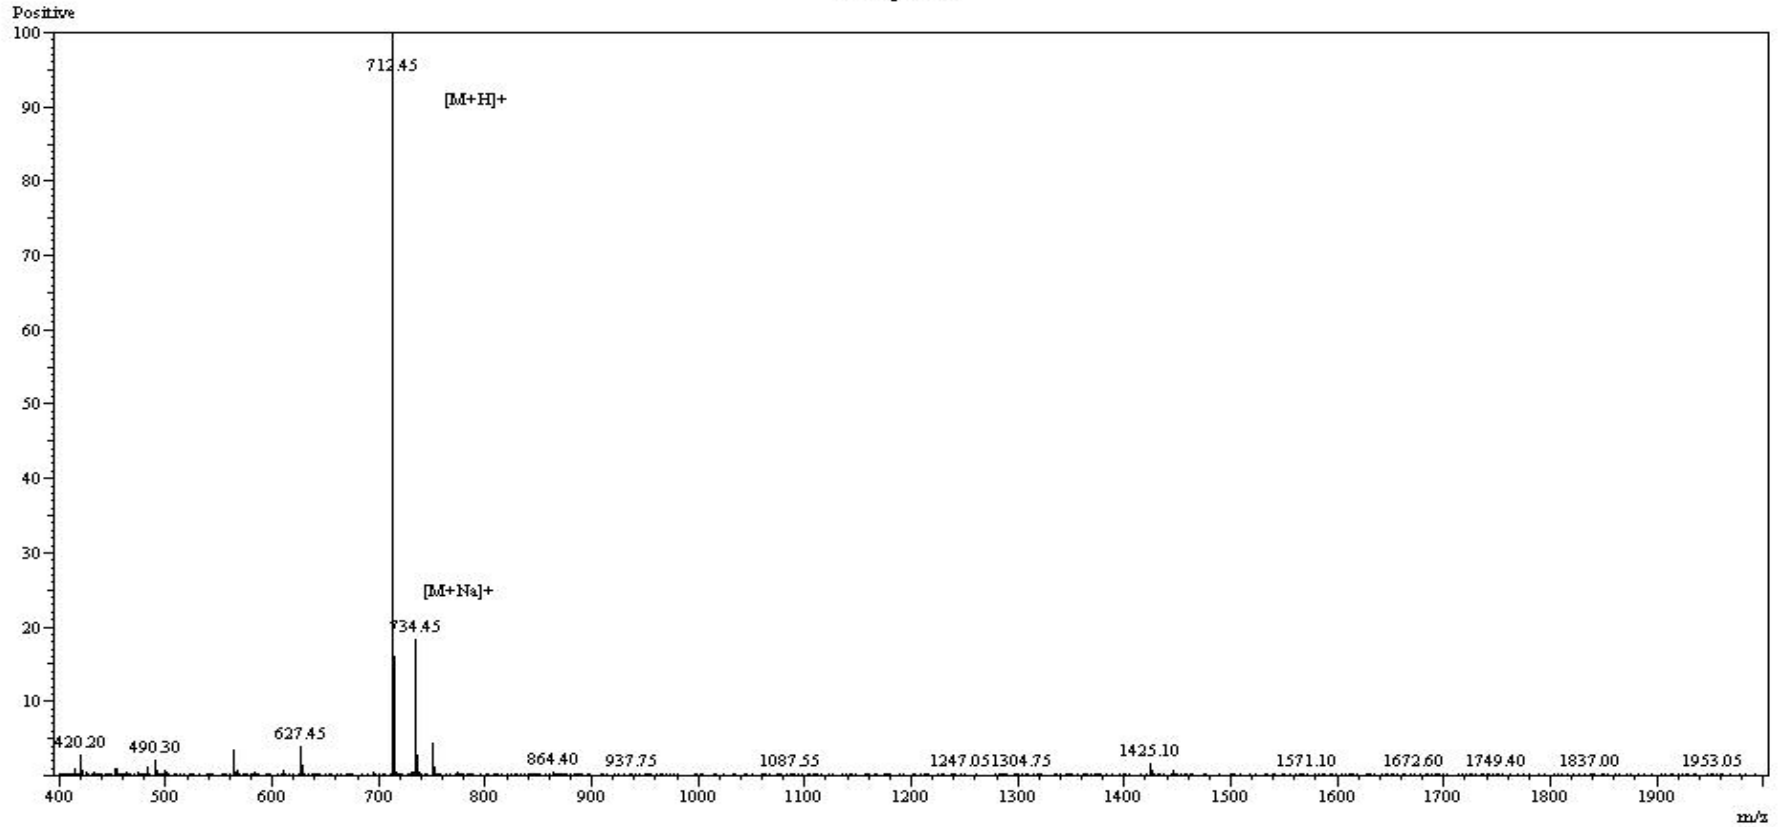

Sample Information  
Date and Time : 2017-2-21  
User : SHAO  
Sample : 488709  
Inj. Volume : 1  
MW : 712.03  
Lot No. : P160811-CQ488709

Probe: ESI  
Nebulizer Gas Flow: 1.5L/min  
CDL: -20.0v  
CDL Temp: 250°C  
Block Temp: 200°C

Probe bias: -3.5kv  
Detector: 1.0kv  
T. Flow: 0.2ml/min  
B. conc: 50%H2O/50%ACN